

FIG. 1

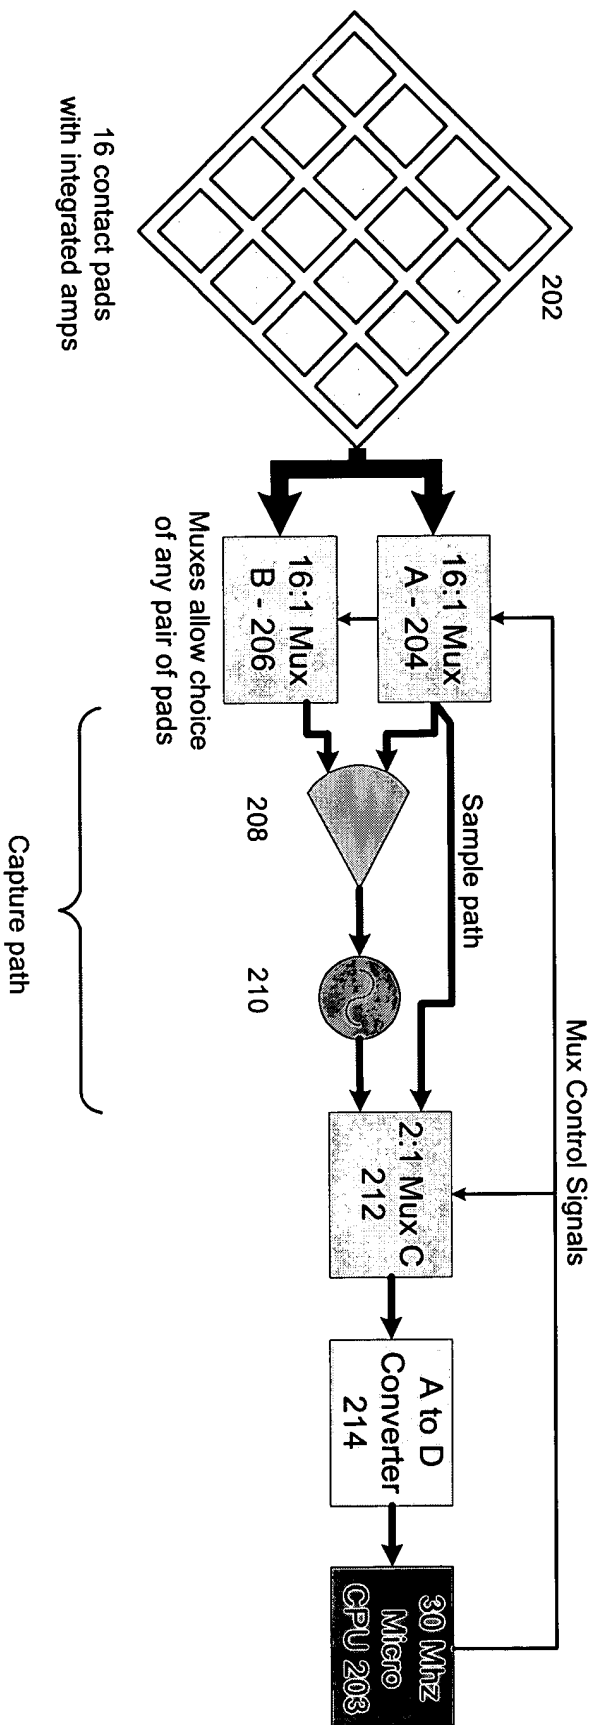


FIG. 2

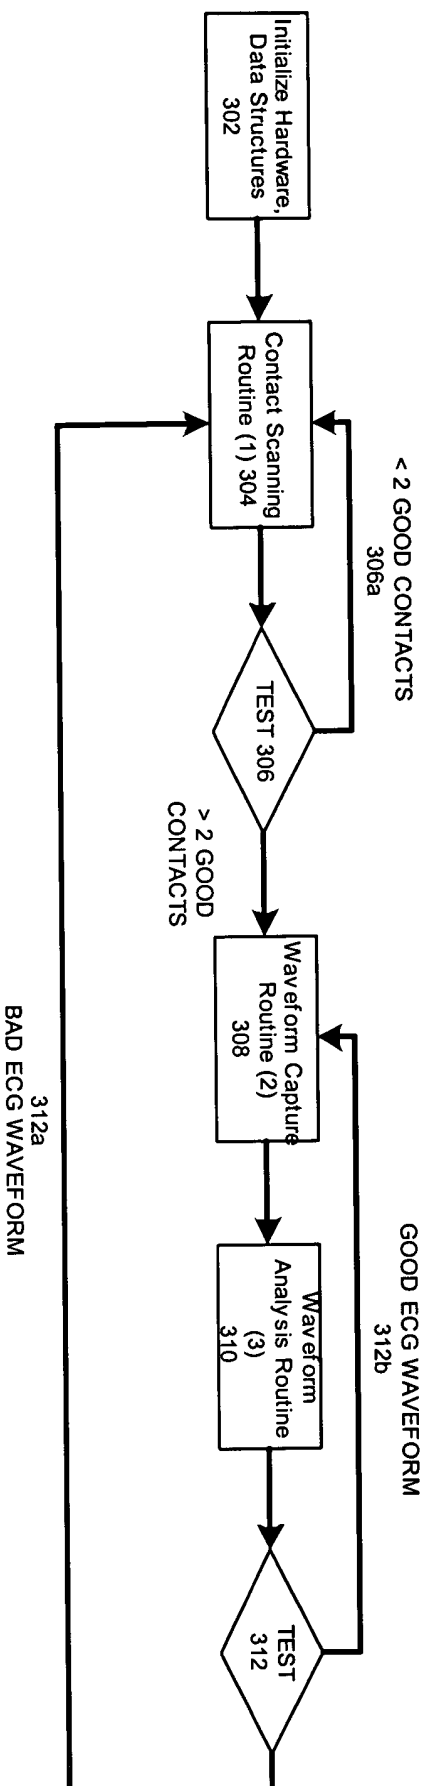


FIG. 3

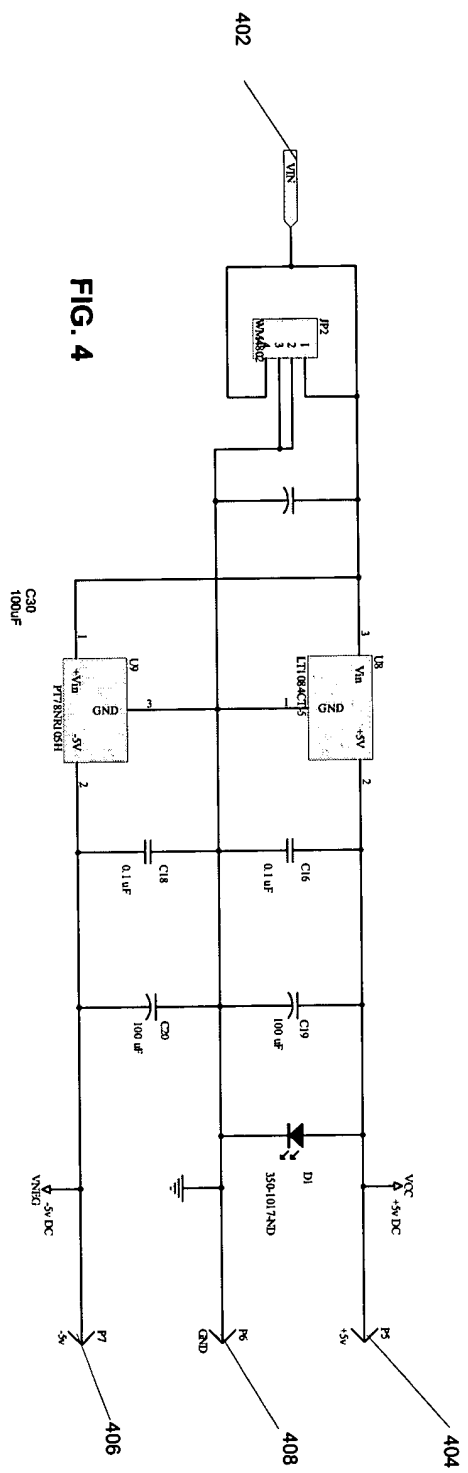
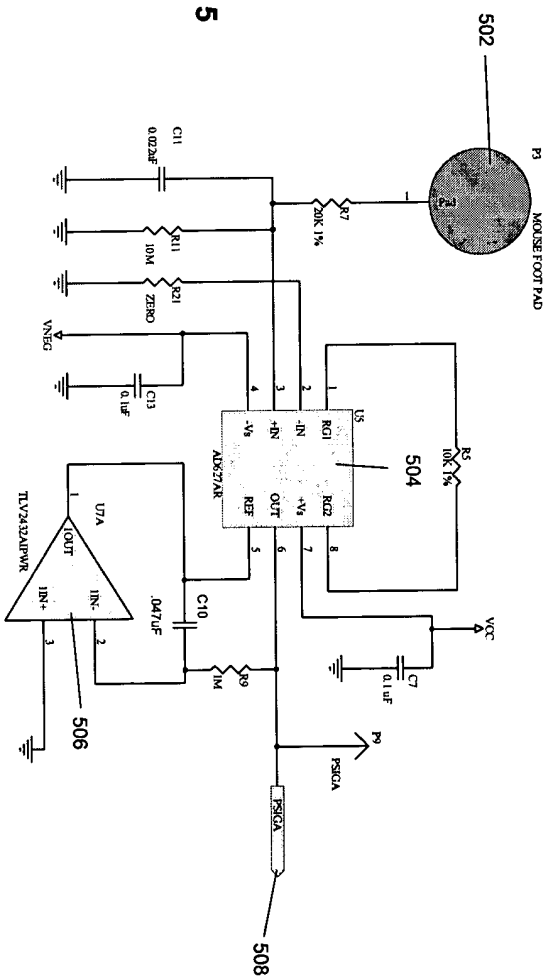
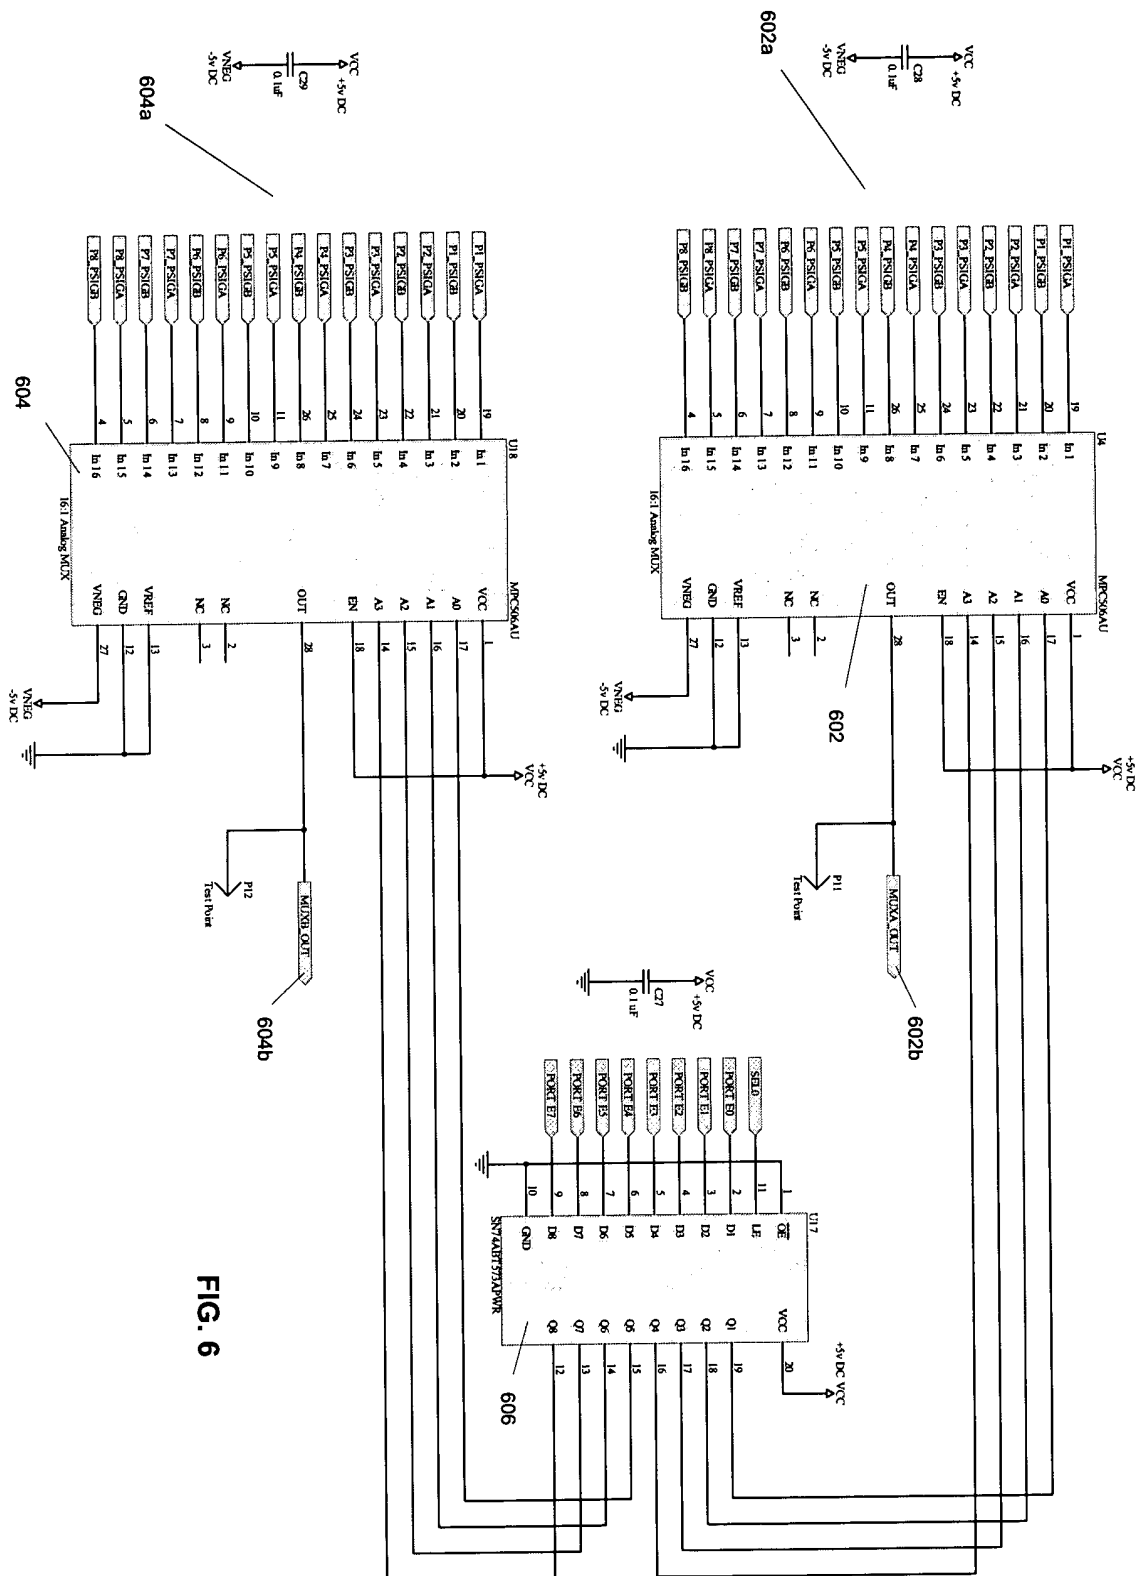
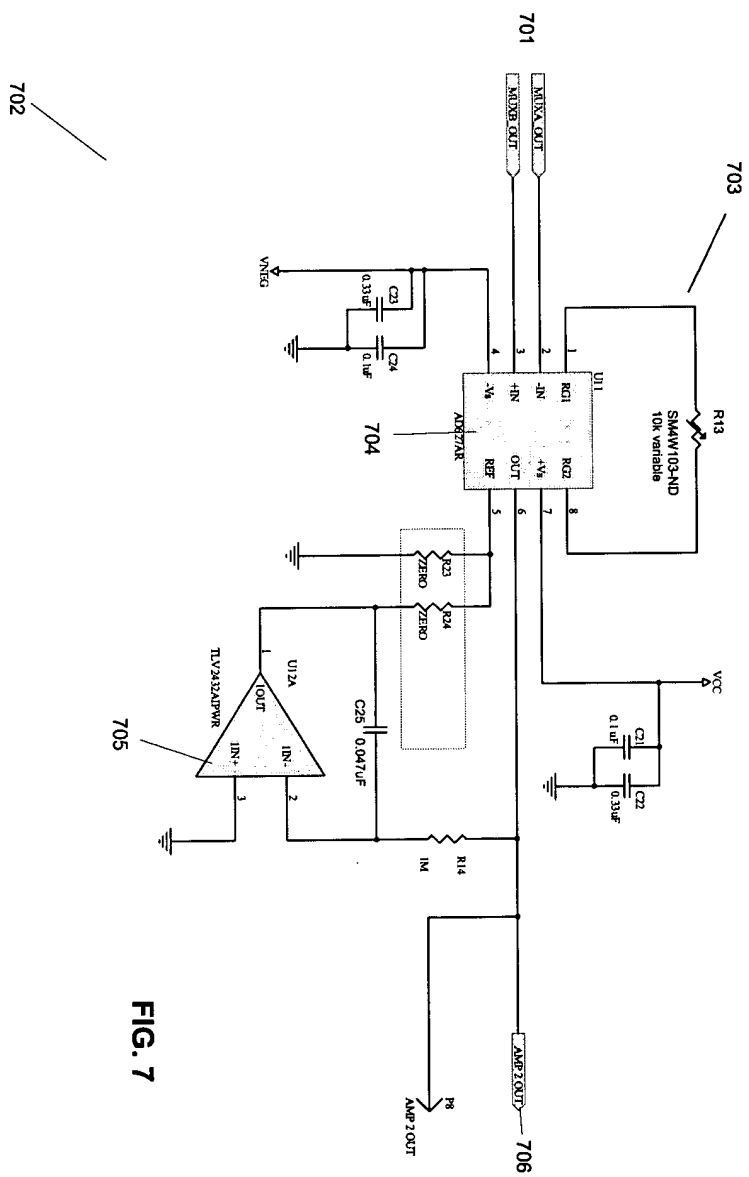


FIG. 4







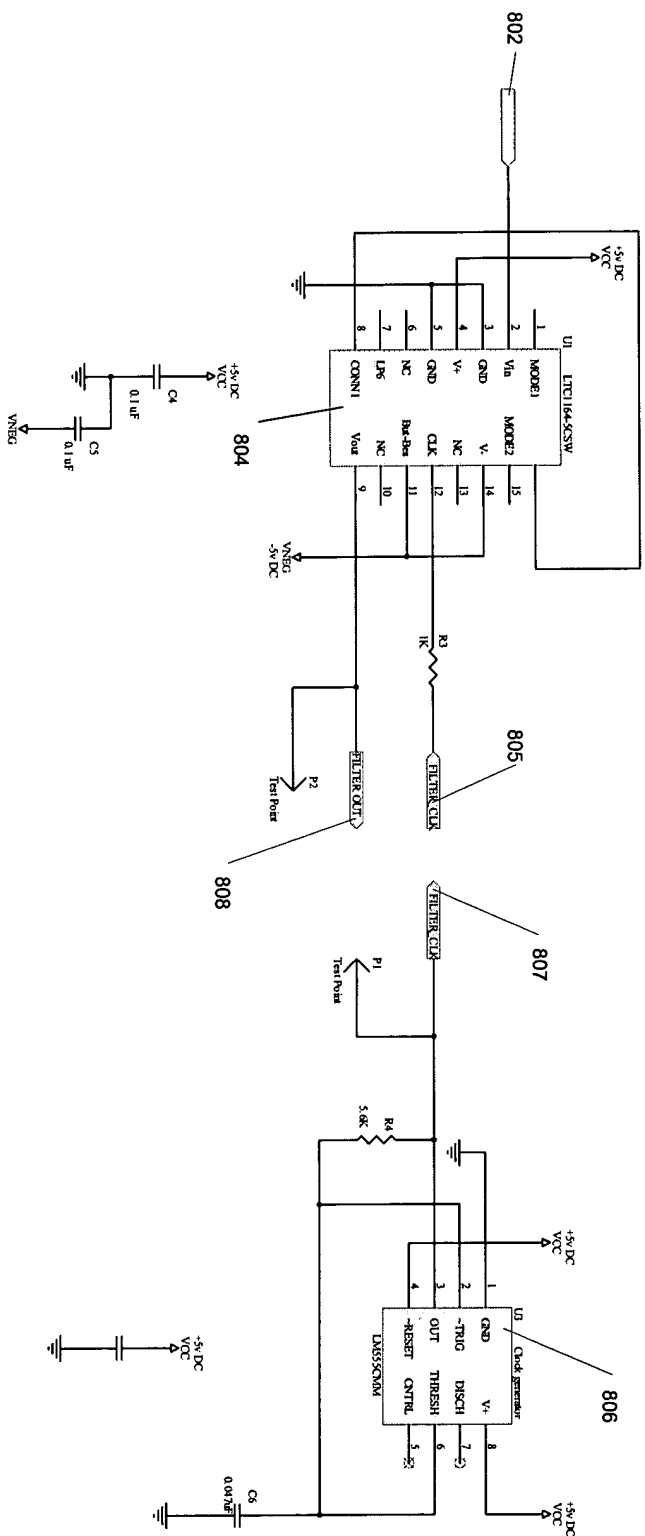


FIG. 8

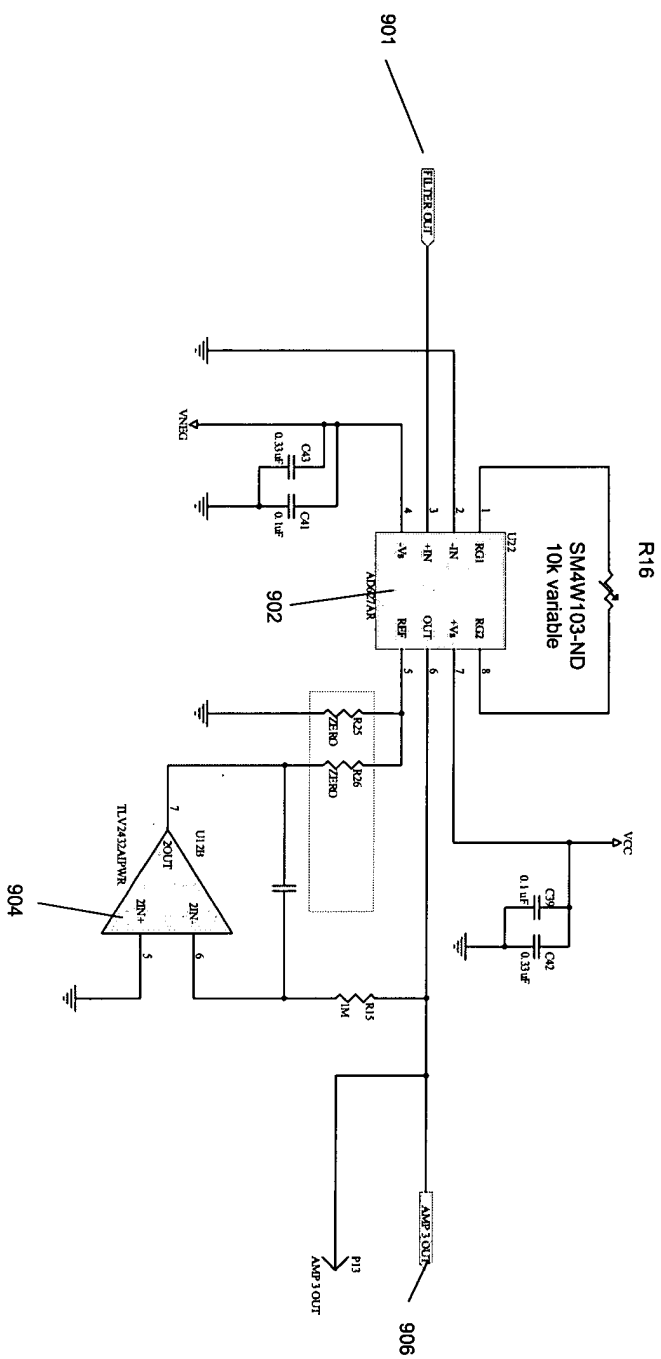


FIG. 9

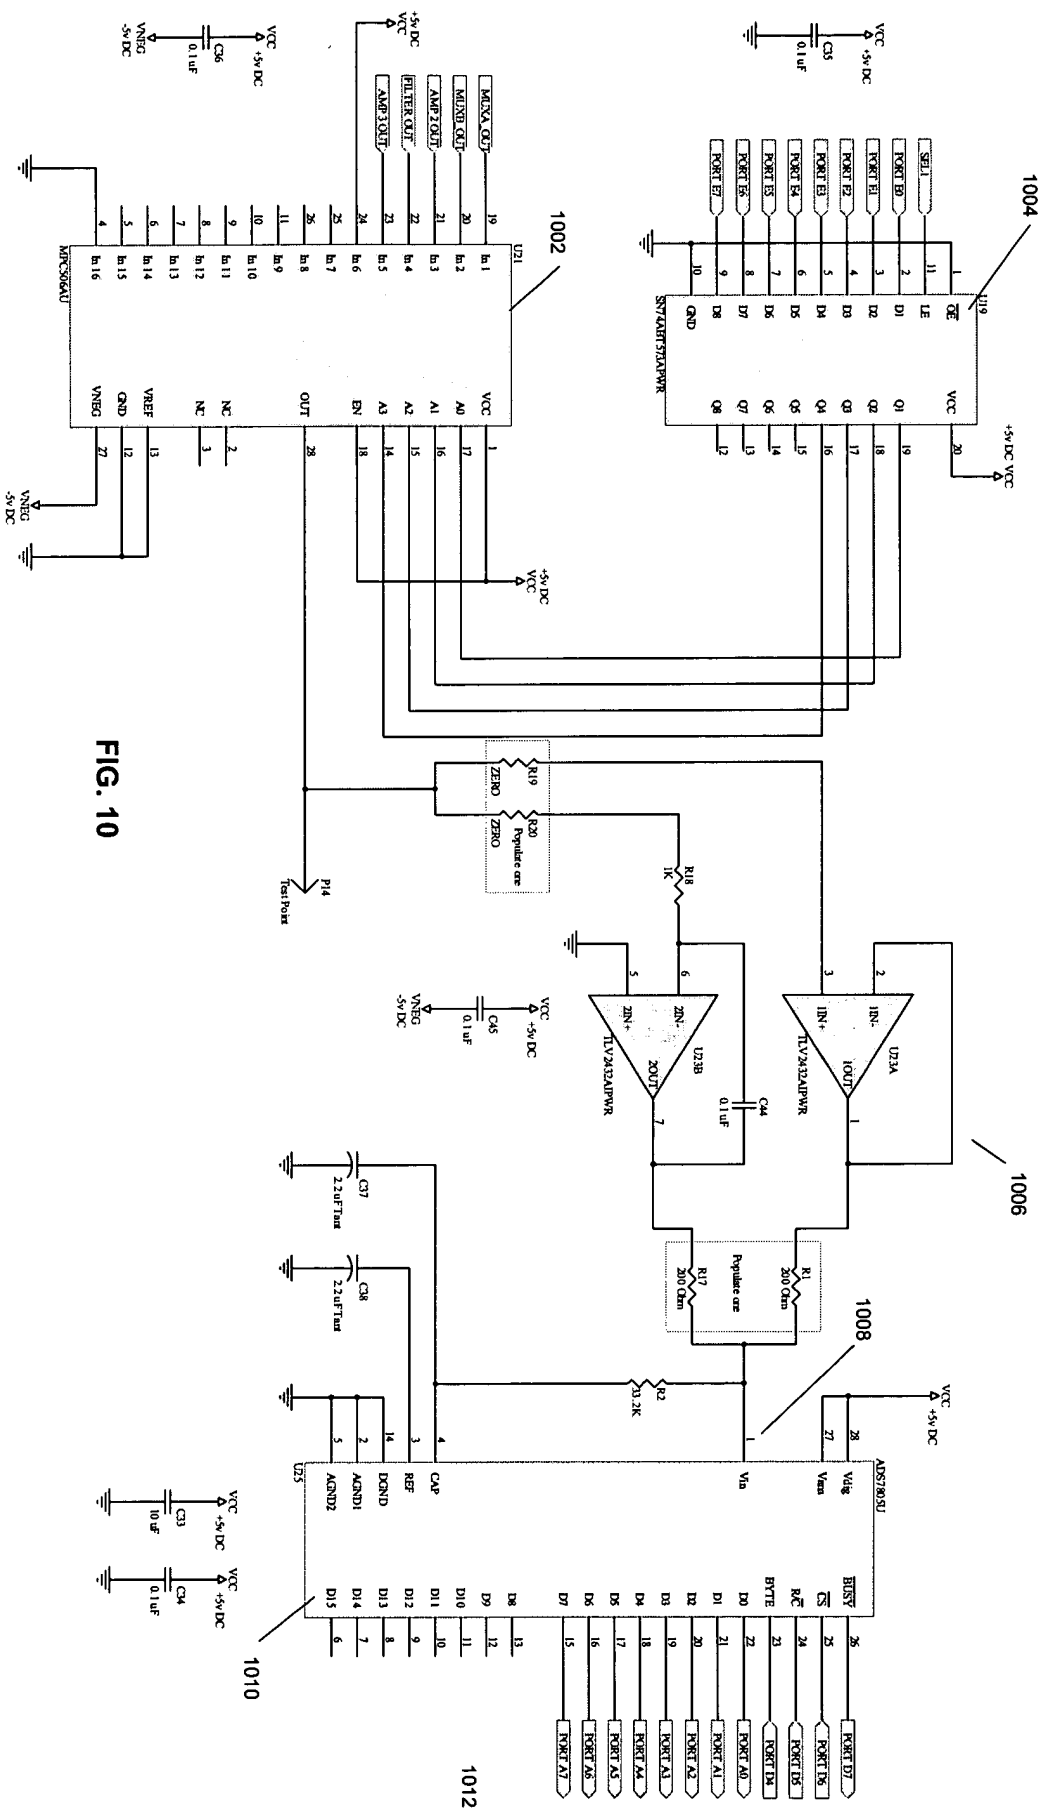


FIG. 10

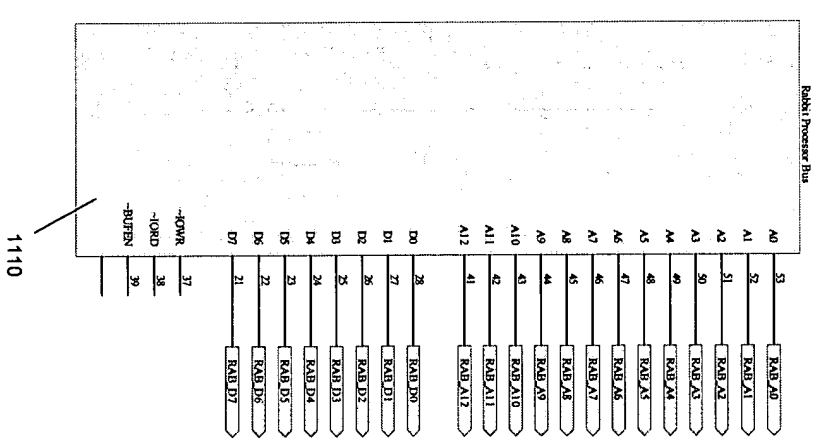
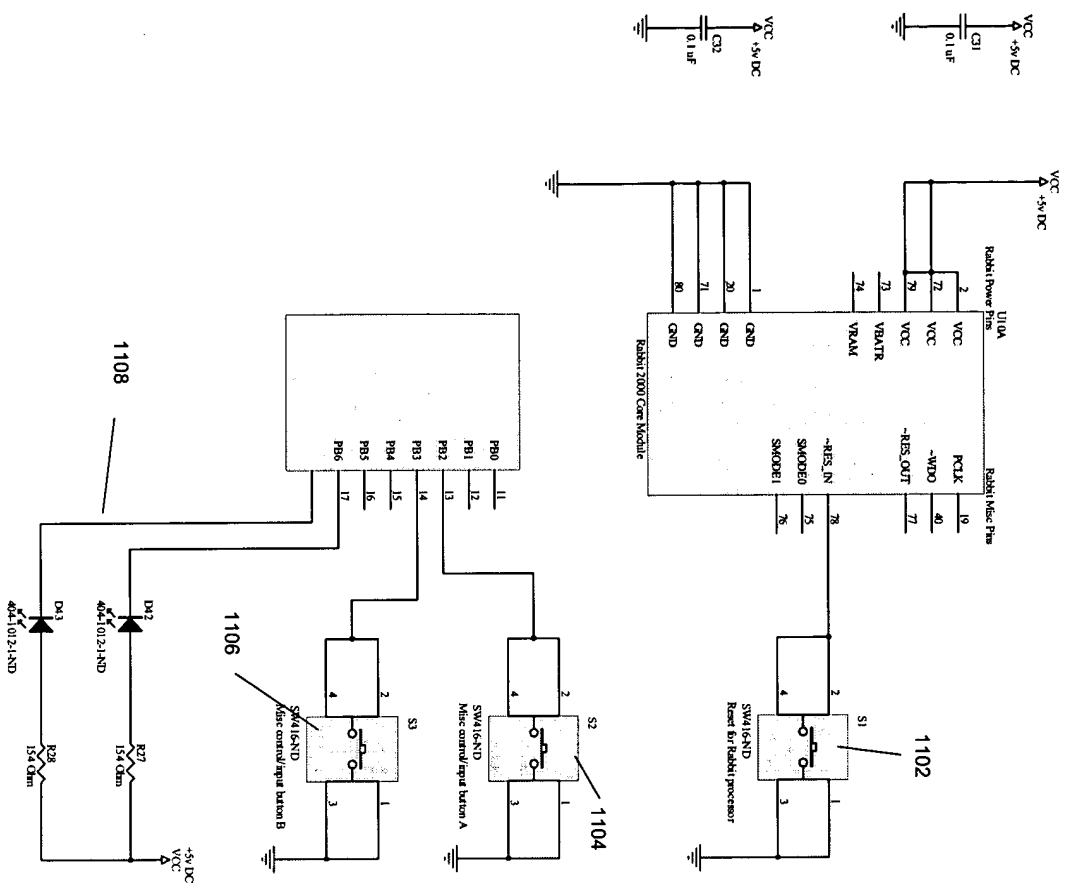


FIG. 11

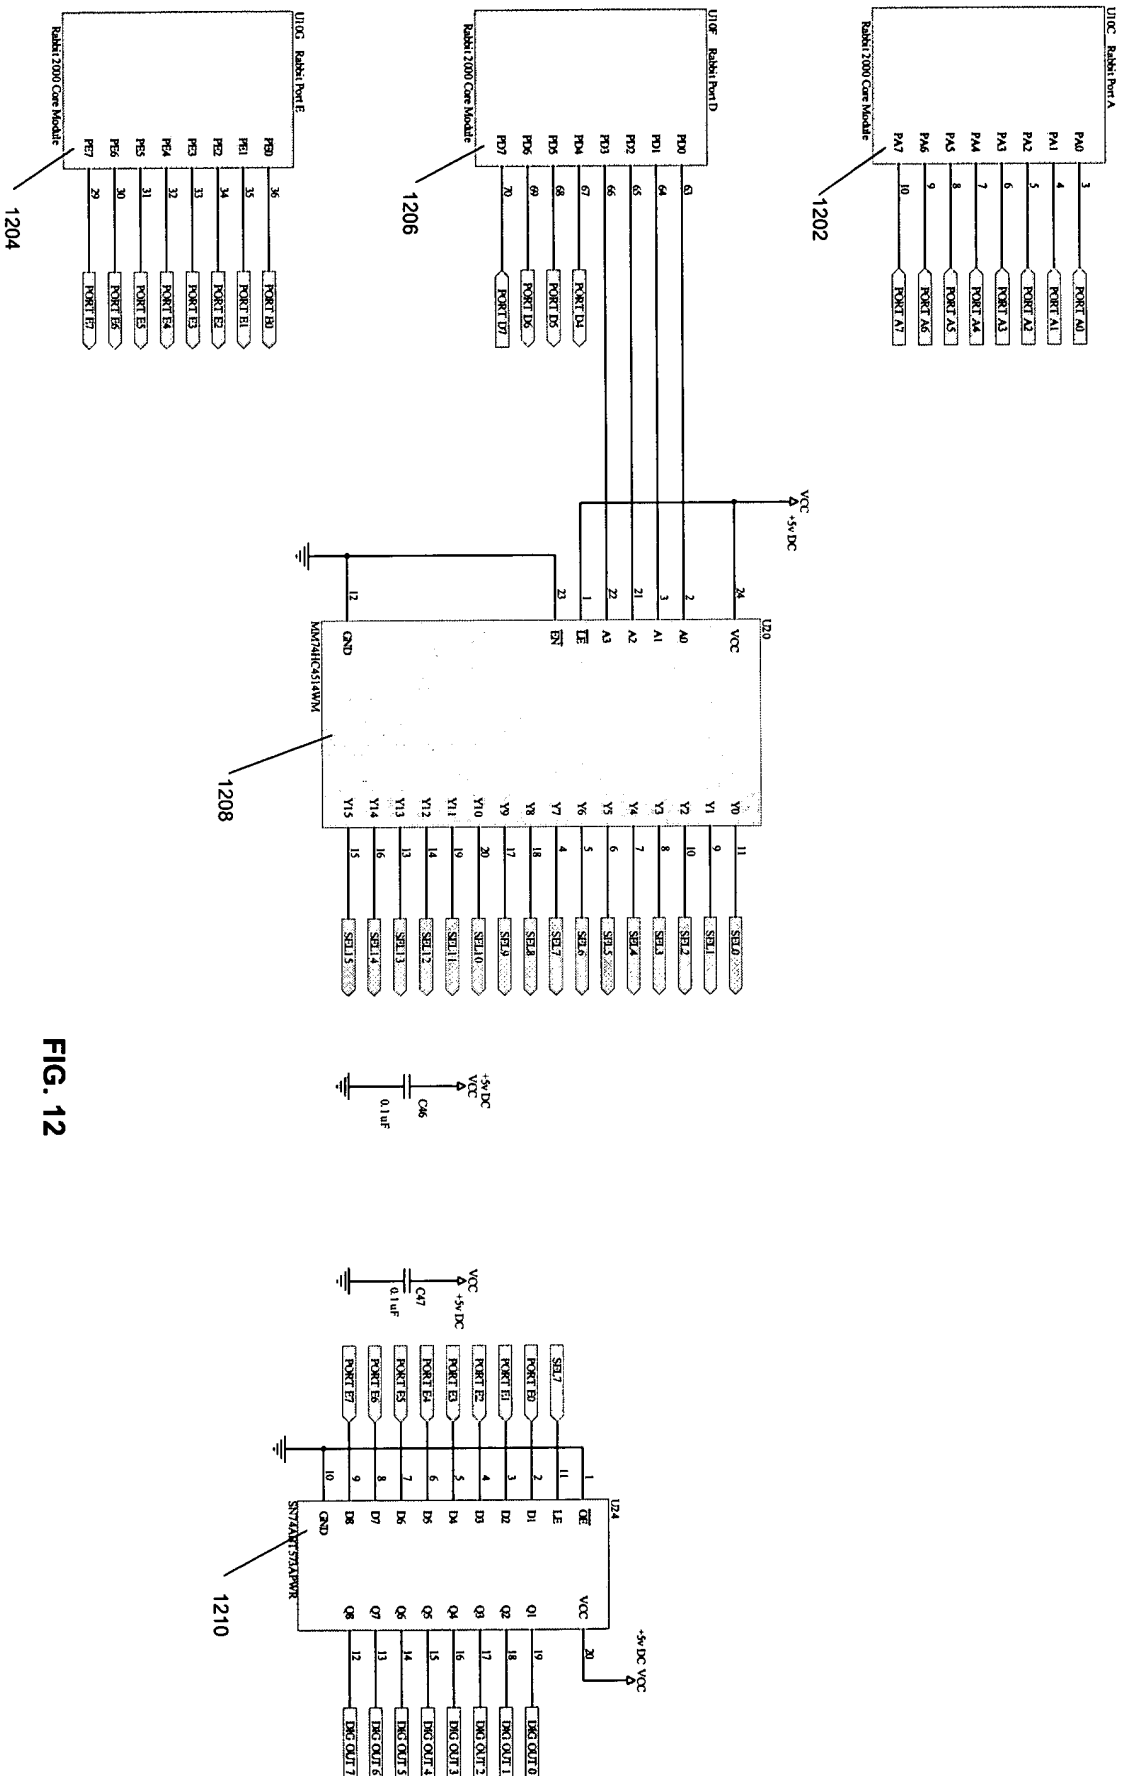


FIG. 12

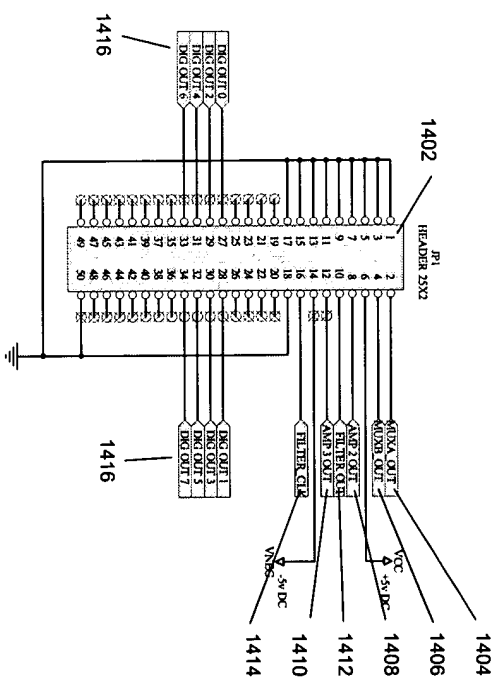
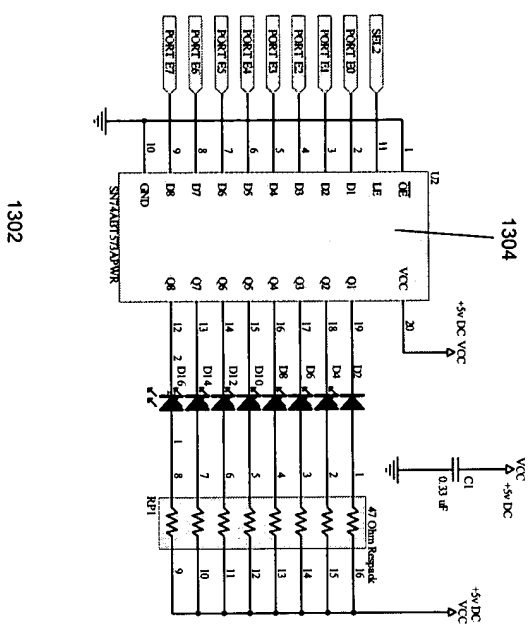


FIG. 15 SmartCube vs Subcutaneous ECG - Avg of 140 Samples

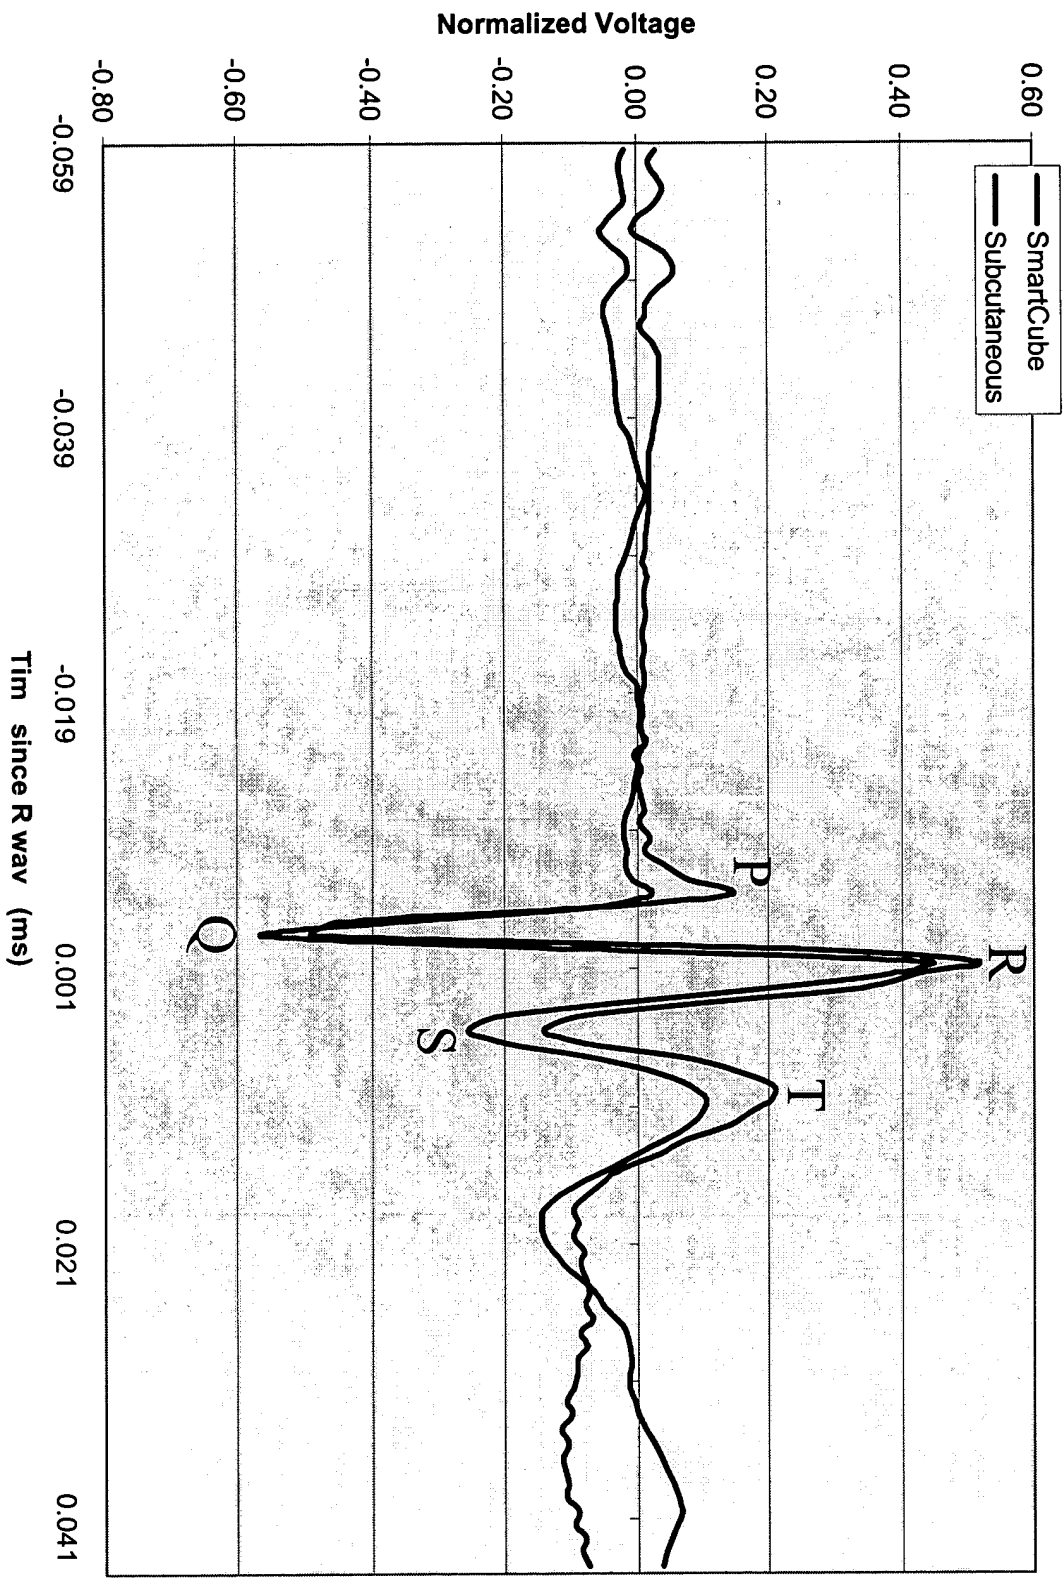


FIG. 16

Mean HR (BPM)

